

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:

DataMaster cdm S/N 130114 ✓

Name Kevin Stevenson

ID# 2114 ✓

Date 12-20-08 ✓

A

Agency UAA Police Dept

Phone # 786 1120

Instrument Location UAA Police Dept (DVI Processing Room) ✓

B

Alco S/N X301591 ✓

Target Value 0.080 ✓

High Pressure 600

Alco Test Value Average 0.080 ✓

1st Alco

0.079 ✓

2nd Alco

Signature [Signature] ✓

CS

12/30/08


Under the Alaska Rules of Evidence, I certify that, (OVER)

(Do Not write in the area below)
(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Kevin Stevenson, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed

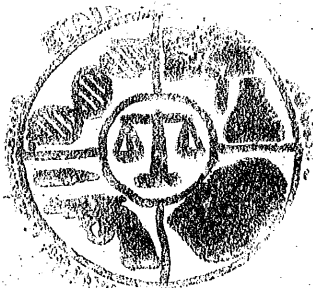

[Signature]

Jeanne Swartz

Scientific Director Designee

State of Alaska

State Breath Alcohol Testing Program

12/31/08

Date

DEC 23 2008

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130114

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130114

DECEMBER 20, 2008

OPERATOR'S NAME:

STEVENSON KEVIN L

OPERATOR'S NUMBER: 2414

SUBJECT'S LAST NAME:

VERIFICATION

SUBJECT'S FIRST NAME/MI :

VERIFICATION

O.L. #: 1234

DEPT/AGENCY: ANC7

CASE/REPORT: 09097

TEST TYPE: U

ALCO TARGET VALUE: .000 ✓

ALCO S/N: K301591

— BREATH ANALYSIS —

.000 ADJUSTED FOR 30.19 in		
ALCO TARGET	.000	23:18
BLANK TEST	.000	23:19
INTERNAL STANDARD	VERIFIED	23:19
ALCO TV 30.19 in	.000 ✓	23:19
BLANK TEST	.000	23:20
SUBJECT SAMPLE	.000	23:20
BLANK TEST	.000	23:21
ALCO TV 30.19 in	.079 ✓	23:22
BLANK TEST	.000	23:22

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130114

DECEMBER 20, 2008

TIME 23:15

— DIAGNOSTIC CHECK —

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	41c
BAROMETER:	30.19 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJKLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~